

FUZIO



6-22

33-39

40-56

57-72

SUBSTRAKTO



KOLOZOMI



ESTUGAMO

INTERVALLO



INTERVALLO

ESTUGAMO

MIN

MIN

MIN

MIN

ESTUGAMO


MAX

MAX

MAX

MAX


ESTUGAMO

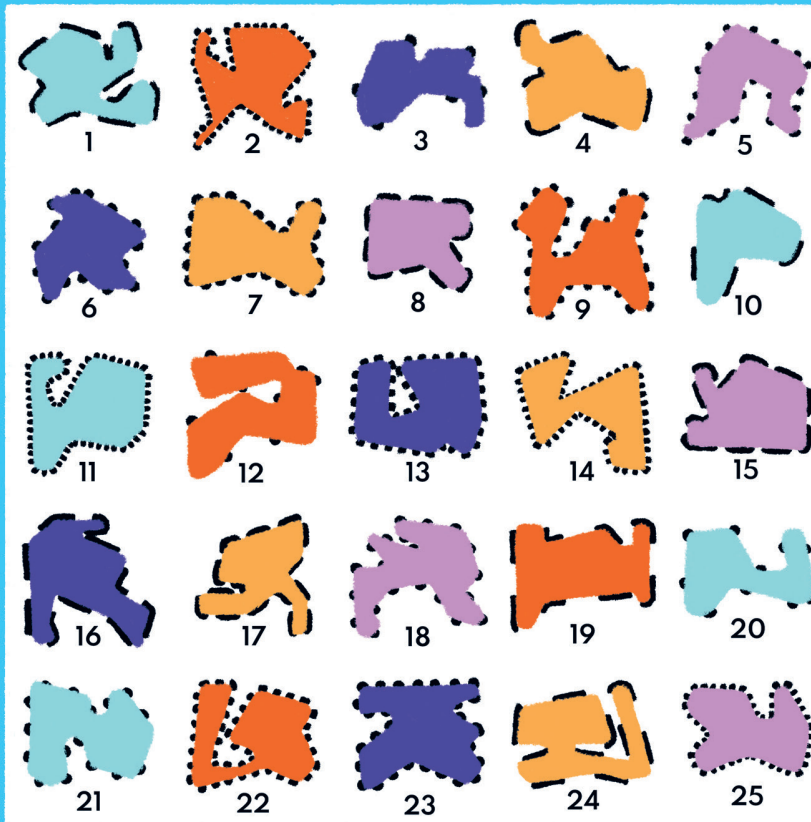

MEZAKOL




SCANPAD



ANTIDOTE



MIKROSKOPO
SAMPLO




CENTRIFUGO



MIKROSKOPO
SAMPLO




x1



ANALYZER

x2



ANALYZER

x3

FUZIO



6-22

33-39

40-56

57-72

SUBSTRAKTO



KOLOZOMI



ESTUGAMO

INTERVALLO



MIN



MIN



MIN



MIN



ESTUGAMO

1 2 3 4 5
6 7 8 9 10
11 12 13 14 15
16 17 18 19 20
21 22 23 24 25

INTERVALLO



MAX



MAX



MAX



MAX



ESTUGAMO

MEZAKOL



SCANPAD



0



1



2



3

ANTIDOTE



0



1



2



3

LAB 1 2 3 4 5 6 7 8 9 10


1 2 3 4 5 6 7 8 9 10

MIKROSKOPO SAMPLY

MIKROSKOPO SAMPLY



CENTRIFUGO



MIKROSKOPO SAMPLY

x1

ANALYZER

x2

ANALYZER

x3